
सामान्य प्रयोजन पैकिंग/लपेटे हुए
कागज — विशिष्टि
(पहला पुनरीक्षण)

**General Purpose Packing/Wrapping
Paper — Specification**
(*First Revision*)

ICS 85.080

© BIS 2021



भारतीय मानक ब्यूरो
BUREAU OF INDIAN STANDARDS
मानक भवन, 9 बहादुरशाह ज़फर मार्ग, नई दिल्ली – 110002
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI-110002
www.bis.gov.in www.standardsbis.in

FOREWORD

This Indian Standard (First Revision) was adopted by the Bureau of Indian Standards, after the draft finalized by the Paper Based Packaging Materials Sectional Committee had been approved by the Chemical Division Council.

This standard was first published in 1972. In this revision the value of burst index has been increased considering Wrapping paper of high GSM Kraft papers are being used in core making. This would lead to good core strength and minimize the core collapse/ crush. It has been observed that if the paper moisture is more, the absorption of glue, a pasting media, is low and the adhesive property will get affected and will yield poor core strength. Considering this and also that the binding property of the wrapping paper depends on the moisture content of the paper, the requirement of moisture has been included. It has also been found that the round discs made of high GSM wrapping paper are used while packing reels. Gum is applied on the outer surface of the round disc. The Cobb with a higher value will cause the applied gum to find its way on to the inside paper which will ultimately cause sticking of paper layers. Therefore, Cobb₆₀ value has been included. Considering the present market trend Packages contain 125 sheets also incorporated in addition to 500 or 250 sheets. This revised version also incorporates all the Amendments issued so far.

A scheme for labelling environment friendly products to be known as ECO Mark has been introduced at the instance of the Ministry of Environment and Forests (MEF). The ECO Mark is administered by the Bureau of Indian Standards (BIS) under the *BIS Act*, 1986 as per the Resolution No. 71 dated 20 February 1991, published in the Gazette of the Government of India. For a product to be eligible for ECO Mark it shall also carry Standard Mark of BIS for quality, in addition to the compliance with the optional environment friendly (EF) requirements. For this purpose, the Standard Mark of BIS would be a single mark being a combination of the ISI Mark and the ECO logo. Requirements to be satisfied for a product to qualify for the BIS Standard Mark for ECO friendliness are included in this Indian Standard. These requirements are optional; manufacturing units will be free to opt for the ISI Mark alone also. It is based on the Gazette Notification No. 364 dated 7 September 1995 for packaging material/package (Part I Paper Board and Plastics Excluding Laminates) as environment friendly products, published in the Gazette of India. This requirement is, therefore, included in this standard to include EF requirements for general purpose packing/wrapping paper.

The composition of the Committee responsible for formulation of this standard is given in Annex C.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2 : 1960 'Rules for rounding off numerical values (*revised*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

Indian Standard

GENERAL PURPOSE PACKING/WRAPPING PAPER — SPECIFICATION

(First Revision)

1 SCOPE

This standard prescribes the requirements and methods of sampling and test for general purpose packing/wrapping paper including the brown wrapping paper.

2 REFERENCES

The standards listed in Annex A contain provisions which through reference in this text, constitute provisions of and necessary adjuncts to this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated in Annex A.

3 TERMINOLOGY

For the purpose of this standard, the definitions given in IS 4661 shall apply.

4 REQUIREMENTS

4.1 General — The paper shall be machine finished or machine glazed. The paper shall be of uniform formation, thickness and substance and shall be evenly finished, free from creases, cuts and holes. It shall also be reasonably free from specks.

4.2 Grammage and Tolerance on Grammage — The nominal grammage shall be as agreed to between the purchaser and supplier. However, when tested as per 6 of IS 1060 (Part 1) no single test result shall vary by more than ± 6 percent from the nominal grammage. Further, mean of 10 test results shall not vary from the nominal by more than ± 4 percent.

4.3 The paper shall also comply the requirements given in Table 1.

4.4 Additional Requirements for ECO Mark

4.4.1 General Requirements

4.4.1.1 The product shall conform to the requirements for quality and performance prescribed under 4.1 to 4.3.

4.4.1.2 The manufacturer shall produce to BIS, the environmental consent clearance from the concerned State Pollution Control Board as per the provisions of *Water (Prevention and Control of Pollution) Act*, 1974 and *Air (Prevention and Control of Pollution) Act*, 1981 along with the authorization, if required under the *Environment (Protection), Act*, 1986 and the Rules made thereunder, while applying for ECO Mark. Additionally the manufacturers shall also comply with the provisions under *Prevention of Food Adulteration Act*, 1954 and the Rules made thereunder wherever necessary.

Table 1 Requirements for General Purpose Packing/Wrapping Paper

(Clause 4.3)

SI No.	Characteristic	Requirement	Method of Test, Ref to Cl No. in IS 1060 (Part 1)
(1)	(2)	(3)	(4)
i)	Burst index, $\text{kPa.m}^2/\text{g}$, <i>Min</i>	1.96	12.5
ii)	Tear index, in both machine and cross direction, $\text{m N.m}^2/\text{g}$, <i>Min</i>	5.88	12.7
iii)	Tensile index, in machine direction, Nm/g , <i>Min</i>	29.4	12.3
iv)	Moisture content, Percent, <i>Max</i>	8	9.0
v)	Cobb ₆₀ , g/m^2 , <i>Max</i> ,		13.2.2
	Top side	40	
	Bottom side	40	
	Burst index = Burst factor $\times$ 0.098		
	Tear index = Tear factor $\times$ 0.098		
	Tensile index = Breaking length $\times$ 0.009		

4.4.2 Specific Requirements

4.4.2.1 The paper and paper boards packaging materials/packages shall be manufactured from the following raw materials:-

- a) 100 percent waste paper or agricultural/industrial wastes;

OR

- b) A minimum of 60 percent by mass of pulp made from materials other than bamboo, hardwood, softwood and reed.

4.4.2.2 The material if used for the packaging of food materials, shall be manufactured from virgin pulp and shall be free from dioxins. Printed surfaces of the paper shall not come into contact with the food and the maximum amounts of contaminants in paper intended to come into contact with food shall not exceed the limits prescribed in Table 2 when tested according to the methods given in Annex B.

5 PACKING AND MARKING

5.1 Packing

5.1.1 A ream of 500 sheets shall be the measure of quantity for wrapping paper in sheets. Packages shall contain 500 or 250 or 125 sheets according to the size and mass of the paper and packed as agreed to between the purchaser and the supplier

5.1.2 Wrapping paper in rolls, shall be rolled on a core of 76 mm inside diameter and in length corresponding to the width of paper, with a wooden plug at each end extending to a minimum of 75 mm into the core.

5.1.3 For ECO Mark, packing/wrapping paper shall be packed in such packages which shall be recyclable/reusable or biodegradable.

5.2 Marking

5.2.1 Each package and roll shall be marked with the following information:

- a) Description and grammage of the material;
- b) Size of paper;

- c) Mass in kg per ream of 500 sheets including wrapping paper; and
- d) Lot number.

5.2.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed there under, and the products may be marked with the Standard Mark.

5.2.3 Additional Requirements for ECO Mark

For ECO Mark, following additional information may also be suitably marked on the container/package:

- a) The criteria base on which the packing/wrapping paper has been labelled as environment friendly a with ECO Mark.
- b) The packing/wrapping paper shall be sold along with instructions for proper use and mode of safe disposal so as to maximize its performance and minimize wastage.
- c) It shall be marked that the ECO-Mark is applicable to the packing/wrapping paper if content is not separately covered under the ECO Mark scheme.

NOTE — It may be stated that the ECO Mark is applicable to the product or packaging material or both.

6 SAMPLING

Representative samples for the test shall be drawn as prescribed in 3 of IS 1060 (Part 1)

7 TEST METHODS

7.1 Tests shall be conducted in accordance with the methods referred to in 4.1, 4.2, Col. 4 of the Table 1 and Annex B.

7.2 Quality of Reagents — Unless specified otherwise, pure chemicals and distilled water (*see* IS 1070) shall be employed.

NOTE — 'Pure chemicals' shall mean chemicals that do not contain impurities which affect the results of analysis.

Table 2 Maximum Permissible Limits of Contaminants in Paper
(Clause 4.4.2.2)

Contaminant	Paper Intended to Come into Contact with Dry Food	Paper Intended to Come into Contact with Wet Food and Food with Fatty Surface	Paper for Filtration
	(mg/kg of paper)	(mg/kg of paper)	(mg/kg of paper)
(1)	(2)	(3)	(4)
Cadmium (Cd)		0.5	0.5
Chromium (Cr ⁶⁺)		0.1	0.1
Lead (Pb)		3.0	3.0
Mercury (Hg)		0.3	0.3
Pentachlorophenol (PCP)	0.05	0.05	0.05
Polychlorinated biphenyls (PCBs)	2.0	2.0	0.5

ANNEX A

(Clause 2)

LIST OF REFERRED INDIAN STANDARDS

<i>IS No.</i>	<i>Title</i>	<i>IS No.</i>	<i>Title</i>
264 : 2005	Nitric acid (<i>third revision</i>)	1060 (Part 3) : 1969	Methods of sampling and test for paper and allied products: Part 3
266 : 1993	Sulphuric Acid (<i>third revision</i>)		
1060 (Part 1) : 1966	Methods of sampling and test for paper and allied products: Part 1 (<i>revised</i>)	1064 : 1980	Specification for paper sizes (<i>second revision</i>)
1060 (Part 2) : 1960	Methods of sampling and test for paper and allied products: Part 2	1070 : 1992	Reagent grade water (<i>third revision</i>)
		4661 : 1999	Glossary of terms used in paper trade and industry (<i>second revision</i>)

ANNEX B

(Clause 4.4.2.2 and Table 2)

DETERMINATION OF CHROMIUM, LEAD, MERCURY, CADMIUM, PENTACHLOROPHENOL AND POLYCHLORINATED BIPHENYLS

B-1 DETERMINATION OF CHROMIUM (AS Cr^{6+})

B-1.1 Principle — The hexavalent chromium is determined colorimetrically by reaction with diphenylcarbazide in acid solution at a wave length of 550 nm.

B-1.2 Apparatus

B-1.2.1 Spectrophotometer — Any spectrophotometer suitable for measurement at a wavelength of about 550 nm or photoelectric absorption meter fitted with filters giving maximum transmission near 550 nm.

B-1.2.2 Shaker — Any shaker suitable for rotating/ moving at 30 ± 2 revolution/min.

B-1.3 Reagents

B-1.3.1 Extraction Fluid — Mix 5.7 ml of acetic acid in distilled water.

B-1.3.2 Nitric Acid — Concentrated (*see* IS 266).

B-1.3.3 Sulphuric Acid — Approximately 0.2 N (*see* IS 264).

B-1.3.4 Diphenylcarbazide Solution — Dissolve 0.25 g of diphenylcarbazide in 50 ml acetone. Store in a brown bottle. Discard when solution becomes discoloured.

B-1.3.5 Stock Chromium Solution — Dissolve 0.141 g $\text{K}_2\text{Cr}_2\text{O}_7$ in distilled water and dilute to 100 ml. One ml of this solution contains 500 μg of chromium (as Cr^{6+}).

B-1.3.6 Intermediate Chromium Solution — Take 10 ml of stock chromium solution and dilute to 1 000 ml with distilled water. One ml of this solution contains 5.00 μg of chromium (as Cr^{6+}).

B-1.3.7 Standard Chromium Solution — Take 10 ml of intermediate chromium solution and dilute to 1 000 ml with distilled water. One ml of this solution contains 0.05 μg of chromium (as Cr^{6+}).

B-1.3.8 Indicator Paper — Covering the pH range 0.5 to 1.5.

B-1.4 Procedure

B-1.4.1 Preparation of Calibration Curve — Into each of a series of ten 250-ml volumetric flasks, place the quantities of standard chromium solution as indicated below:

Standard Chromium Solution	Corresponding to Cr ⁶⁺
ml	µg
1.0	0.05
2.0	0.10
3.0	0.15
4.0	0.20
5.0	0.25
6.0	0.30
7.0	0.35
8.0	0.40
9.0	0.45
10.0	0.50

B-1.4.1.1 Add sulphuric acid to adjust the solution pH to 1.0 ± 0.3 in each flask and dilute to 100 ml. Add 2.0 ml diphenylcarbazide solution, mix thoroughly and wait for 10 minutes.

B-1.4.1.2 Carry out the measurement on the spectrophotometer or on a photoelectric colorimeter using appropriate filter with a 1 cm cell at a wavelength of 550 nm. As references use extraction fluid. Correct the absorbance readings of standard solution by subtracting absorbance of a reagent blank carried through the above method.

B-1.4.1.3 Construct a calibration curve by plotting corrected absorbance values against chromium content in microgram per 102 ml.

B-1.4.2 Determination

B-1.4.2.1 Sample preparation — Tear the air dry sample into pieces of suitable size. Do not use cut or punched edges or other parts where metallic contamination may have occurred.

B-1.4.2.2 Preparation of test solution — Weigh to the nearest 0.01 g about 20 g of paper, leach the paper with about 200 ml of extraction fluid for 18 ± 2 h using shaker rotating/moving at 30 ± 2 rev/min. Filter the extract through glass fibre filter with 0.45 micron pore size. Add sufficient amount of aluminium sulphate and filter if any precipitate appears. Transfer the solution quantitatively to a volumetric flask of suitable capacity, dilute to the mark and mix well.

B-1.4.2.3 According to the expected chromium content, take an aliquot portion of the test solution containing 10 to 100 µg of chromium to a 100-ml volumetric flask. Adjust the pH of the solution to 1.0 ± 0.3 by adding 0.2 N sulphuric acid. Dilute to 100 ml. Add 2 ml diphenylcarbazide solution, mix thoroughly, and wait for 10 minutes.

B-1.4.2.4 Photometric measurement — Carry out the photometric measurements of the test solution according to the methods given in B-1.4.1.1.

B-1.4.3 Calculation — By means of the calibration curve (see B-1.4.1.3) determine the quantity of chromium present:

$$\text{Chromium (as Cr}^{6+}\text{), ppm} = \frac{m \times D}{M}$$

where

m = mass of chromium determined in the aliquot of the sample solution, µg;

M = mass of paper sample taken for testing, g; and

D = ratio of the volume of test solution to the volume of aliquot portion taken for the colour development.

B-2 DETERMINATION OF MERCURY (AS HG)

B-2.1 Principle

The flameless atomic absorption procedure is a physical method based on the absorption of radiation at 253.7 nm by mercury vapour. The mercury is reduced to the elemental state and aerated from solution in a closed system. The mercury vapour passes through a cell positioned in the light path of mercury hollow cathode lamp of an atomic absorption spectrophotometer. Absorbance (peak height) is measured as a function of mercury concentration and record.

B-2.2 Apparatus

B-2.2.1 Atomic Absorption Spectrometer (AAS) and Associated Equipment — Instrument settings recommended by the manufacturer shall be followed. Instruments designed specifically for the measurement of mercury using the cold vapour technique may be substituted for the AAS.

B-2.2.2 Mercury Vapour Generation Assembly — Consists of an absorption cell, peristaltic pump, flow meter, aeration tubing and a drying tube containing magnesium perchlorate.

B-2.2.3 Mercury Hollow Cathode Lamp

B-2.2.4 Recorder/Printer/Display Meter — Any multi-range variable recorder that is compatible with the UV detection system is suitable.

B-2.3 Reagents

B-2.3.1 Sulphuric Acid — Concentrated (see IS 266).

B-2.3.2 Nitric Acid — Concentrated (see IS 264).

B-2.3.3 Stannous Chloride Solution — Dissolve 25 g of stannous chloride (SnCl₂) in water containing 50 ml of concentrated hydrochloric acid and dilute to 250 ml. If a suspension forms, stir reagent continuously during use.

B-2.3.4 Sodium Chloride — Hydroxylamine Sulphate Solution — Dissolve 12 g of sodium chloride and 12 g of hydroxylamine sulphate $(\text{NH}_2\text{OH})_2 \text{H}_2\text{SO}_4$ in distilled water and dilute to 100 ml.

B-2.3.5 Potassium Permanganate Solution — Dissolve 5 g of potassium permanganate in distilled water and dilute to 100 ml.

B-2.3.6 Potassium Persulphate Solution — Dissolve 5 g of potassium persulphate in distilled water and dilute to 100 ml.

B-2.3.7 Stock Mercury Solution — Dissolve 1.354 g of mercuric chloride in about 700-ml of distilled water. Add 10-ml of concentrated nitric acid and make up to 1 000 ml. One millilitre of the solution contains 1 mg of mercury as Hg.

B-2.3.8 Standard Mercury Solution — Prepare a series of standard mercury solutions containing 0 to 5 $\mu\text{g/l}$ by appropriate dilution of stock mercury solution (B-2.3.7) with water containing 10 ml of concentrated nitric acid per litre. Prepare standards daily.

NOTE — Use mercury free distilled water for the preparation of reagents and standards.

B-2.4 Procedure

B-2.4.1 Instrument Operation — Follow the procedure of the manufacturer's operating manual. Connect the mercury vapour generating assembly as shown in Fig. 1.

B-2.4.2 Standardization — Transfer 100 ml of each of the 1.0, 2.0 and 5.0 $\mu\text{g/l}$ standard mercury solution and a blank of 100 ml water to 300 ml BOD bottles. Add 5 ml of concentrated sulphuric acid and 2.5 ml of concentrated nitric acid to each bottle. Add 15 ml of potassium permanganate solution to each bottle and let stand for at least 15 min. Add 8-ml of potassium persulphate $(\text{K}_2\text{S}_2\text{O}_8)$ solution to each bottle and heat for 2 h in a water bath at 95 °C. Cool and add 6 ml of sodium chloride-hydroxylamine sulphate solution to reduce the excess permanganate. After decolourization add 5 ml of stannous chloride solution and attach the bottle immediately to the aeration apparatus forming a closed system. As mercury is volatilised and carried into the absorption cell, absorbance will increase to a maximum within a few seconds. As soon as recorder returns approximately to the base line, remove stopper holding the aeration frit from the reaction bottle and replace with a bottle containing distilled water. Flush the system for a few seconds and run the next standard in the same manner. Construct a standard calibration curve by plotting absorbance (peak height) versus mercury concentration in μg .

B-2.4.3 Determination

B-2.4.3.1 Sample preparation — Tear the air dry sample into pieces of suitable size. Do not use cut or punched edges or other parts where metallic contamination may have occurred.

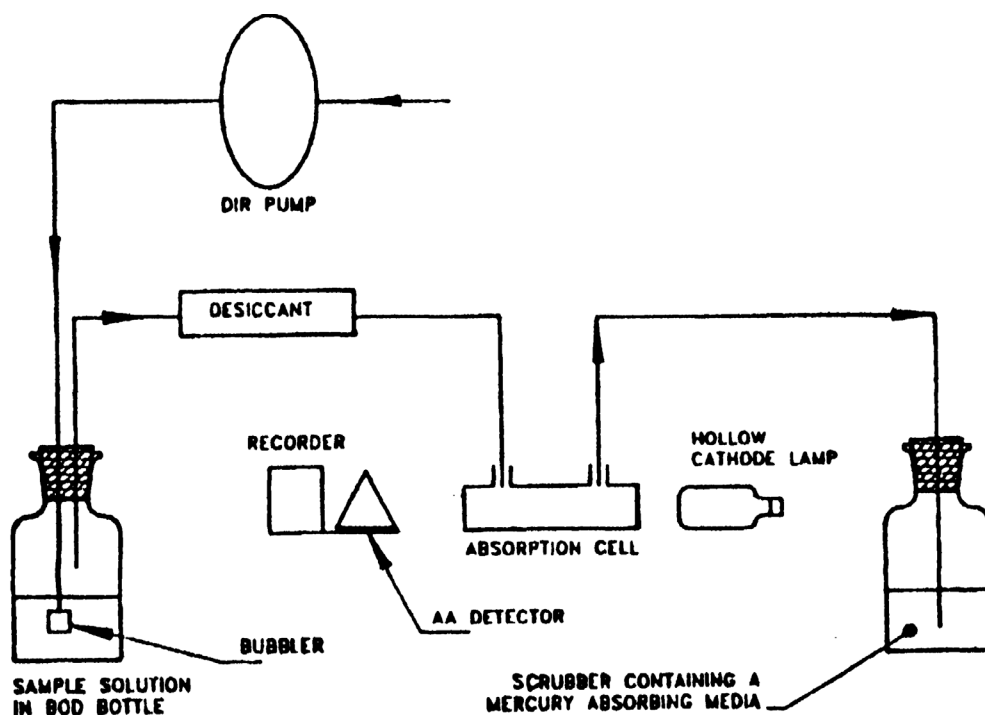


FIG.1 SCHEMATIC ARRANGEMENT OF EQUIPMENT FOR MEASUREMENT OF MERCURY BY COLD VAPOUR ATOMIC ABSORPTION TECHNIQUE

B-2.4.3.2 Preparation of test solution — Weigh to the nearest 0.01 g about 20 g of paper, leach the paper with about 200 ml of extraction fluid for 18 ± 2 h using shaker rotating/moving at 30 ± 2 rev/min. Filter the extract through glass fibre filter with 0.45 micron pore size. Transfer the solution quantitatively to a volumetric flask of suitable capacity, dilute to the mark and mix.

B-2.4.3.3 According to the expected mercury content, take an aliquot portion of the test solution containing not more than 5 µg/l of mercury to a 300-ml BOD bottle and treat as in B-2.4.2.

B-2.5 Calculation

Determine peak height of sample from recorder chart, read mercury value from standard curve and determine the mercury content of the sample using the following formula:

$$\text{Mercury (as Hg), ppm} = \frac{C \times V}{M \times 1000}$$

where

C = concentration of mercury from the calibration curve;

V = volume of test solution prepared, ml; and

M = mass of paper sample taken for testing; g.

B-3 DETERMINATION OF LEAD (AS PB)

B-3.1 Principle

The lead content of the sample is determined by electro thermal atomic absorption spectrometric method.

B-3.2 Apparatus

B-3.2.1 Atomic Absorption Spectrometer — With graphite oven technique in place of conventional burner assembly.

B-3.2.2 Lead Hollow-Cathode Lamp or Multielement Hollow-Cathode Lamp — For use at 283.3 nm.

B-3.2.3 Hot Plate

B-3.3 Reagents

B-3.3.1 Nitric Acid — Concentrated (see IS 264).

B-3.3.2 Nitric Acid — 1 : 1.

B-3.3.3 Dilute Nitric Acid — 1 : 499.

B-3.3.4 Stock Lead Solution — Dissolve 1.599 9 g of $\text{Pb}(\text{NO}_3)_2$ in a mixture of 10 ml of concentrated NO_3 and 100 ml of water and dilute to 1 litre. One ml of this solution contains 1.0 mg of lead (as Pb).

B-3.3.5 Intermediate Lead Solution

B-3.3.6 Standard Lead Solution — Dilute 100 ml of intermediate lead solution to 1 litre with dilute nitric

acid (1 : 499). One milliliter of this solution contains 0.1 mg of lead (as Pb).

B-3.4 Procedure

B-3.4.1 Sample Preparation — Tear the air dry sample into pieces of suitable size. Do not use cut or punched edges or other parts where metallic contamination may have occurred.

B-3.4.2 Preparation of Test Solution — Weigh to the nearest 0.01 g about 20 g of paper, leach the paper with about 200-ml of extraction fluid for 18 ± 2 h using shaker rotating/ moving at 30 ± 2 rev/min. Filter the extract through glass fibre filter with 0.45 micron pore size.

B-3.4.3 Transfer the extract to a 250 ml conical flask. Add 5 ml concentrate nitric acid and a few boiling chips or glass beads. Slowly evaporate on a hot plate to about 10 to 20 ml. Continue heating and adding concentrated nitric acid until digestion is complete. Wash down with water and then filter if necessary. Quantitatively transfer filtrate to a 100 ml volumetric flask, dilute to the mark and mix thoroughly.

B-3.4.4 Inject a measured portion of the digested solution into the graphite oven. Dry, char and atomize according to the preset programme. Measure the absorbance.

B-3.4.5 Prepare a reagent blank and sufficient standards containing 5.0, 7.5 and 10.0 mg/l of lead by diluting suitable volume of the standard lead solution with nitric acid (1 : 499) and repeat as above (B-3.4.3). Inject a suitable portion of each standard solution in order of increasing concentration. Analyze each standard solution and measure the absorbances.

B-3.4.6 Calculation — Construct a standard calibration graph by plotting the absorbance versus mg of lead concentration of each standard. Read the concentration of the sample from the graph and determine the lead content of the sample from the calibration graph using the following formula:

$$\text{Lead (as Pb), ppm} = \frac{C \times F \times 100}{M}$$

where

C = concentration of lead from the calibration curve;

F = dilution factor; and

M = mass of paper sample taken for testing, g.

B-4 DETERMINATION OF CADMIUM (AS CD)

B-4.1 Principle — The cadmium content of the sample is determined by electro thermal atomic absorption spectrometric method.

B-4.2 Apparatus

B-4.2.1 Atomic Absorption Spectrometer — With graphite oven technique in place of conventional burner assembly.

B-4.2.2 Cadmium Hollow — Cathode Lamp or Multielement Hollow-Cathode Lamp — For use at 228.8 nm.

B-4.2.3 Hot Plate

B-4.3 Reagents

B-4.3.1 Nitric Acid — Concentrated (*see* IS 264).

B-4.3.2 Nitric Acid — 1 : 1.

B-4.3.3 Dilute Nitric Acid — 1 : 499.

B-4.3.4 Stock Cadmium Solution — Dissolve 1.0 g of pure cadmium metal in minimum quantity of concentrated nitric acid and dilute to 1 litre with distilled water. One millilitre of this solution contains 1 mg of cadmium (as Cd).

B-4.3.5 Intermediate Cadmium Solution — Add 1 ml of concentrated nitric acid to 50 ml of stock solution and dilute to 1 litre with distilled water. One ml of this solution contains 50 µg of cadmium (as Cd).

B-4.3.6 Standard Cadmium Solution — To 10 ml of cadmium intermediate solution add 1 ml of concentrated nitric acid and dilute to 1 litre with distilled water. One ml of this solution contains 0.5 µg of cadmium (as Cd).

B-4.4 Procedure

B-4.4.1 Sample Preparation — Tear the air dry sample into pieces of suitable size. Do not use cut or punched edges or other parts where metallic contamination may have occurred.

B-4.4.2 Preparation of Test Solution — Weigh to the nearest 0.01 g about 20 g of paper, leach the paper with about 200 ml of extraction fluid for 18 ± 2 h using shaker rotating/moving at 30 ± 2 rev/min. Filter the extract through glass fibre filter with 0.45 micron pore size.

B-4.4.3 Transfer the extract to a 250 ml conical flask. Add 5 ml concentrate nitric acid and a few boiling chips or glass beads. Slowly evaporate on a hot plate to about 10 to 20 ml. Continue heating and adding concentrated nitric acid until digestion is complete. Wash down with distilled water and then filter if necessary. Quantitatively transfer filtrate to a 100 ml volumetric flask, dilute to the mark and mix thoroughly.

B-4.4.4 Inject a measured portion of the digested solution into the graphite oven. Dry, char and atomize according to the preset programme. Measure the absorbance.

B-4.4.5 Prepare a reagent blank and sufficient standards containing 5.0, 7.5 and 10.0 mg/l of cadmium by diluting suitable volume of the standard cadmium solution with nitric acid (1 : 499). Inject a suitable portion of each standard solution in order of increasing concentration. Analyze each standard solution and measure the absorbances.

B-4.4.6 Calculation — Construct a standard calibration graph by plotting the absorbance versus mg of cadmium concentration of each standard. Read the concentration of the sample from the graph and determine the cadmium content of the sample from the calibration graph using the following formula:

$$\text{Cadmium (as Cd), ppm} = \frac{C \times F \times 100}{M}$$

where

C = concentration of cadmium from the calibration curve;

F = dilution factor; and

M = mass of paper sample taken for testing, g.

B-5 DETERMINATION OF PENTACHLOROPHENOL (PCP)**B-5.1 Principle**

PCP is extracted with acetone by Soxhlet extraction. Acetone extract is evaporated to dryness and subjected to acetylation. The acetylated PCP is determined quantitatively by Gas Chromatograph-Electron Capture Detector (GC-ECD).

B-5.2 Apparatus

B-5.2.1 Round Bottom Flask — 250 ml.

B-5.2.2 Soxhlet Extractor

B-5.2.3 Water Bath

B-5.2.4 Separating Funnels — 60 ml and 100 ml.

B-5.2.5 Injection Syringes — 1 µl, 5 µl and 10 µl.

B-5.2.6 Gas Chromatograph with ECD — Capillary columns.

B-5.2.7 Glass Columns — Length 20 cm, internal diameter 12 mm filled with 5 cm of silica gel having particle size $63 \mu\text{m} \times 200 \mu\text{m}$.

B-5.3 Reagents

B-5.3.1 Acetone

B-5.3.2 n-Hexane

B-5.3.3 Acetic Anhydride

B-5.3.4 Sodium Sulphate Anhydrous

B-5.3.5 PCP Stock Solution — Dissolve 10 mg of pentachlorophenol in 100 ml of acetone. One millilitre of this solution contains 0.1 mg of pentachlorophenol.

B-5.3.6 PCP Standard Solution — Dilute 10 ml of stock solution with acetone to 100 ml. One millilitre of this solution contains 0.01 mg of pentachlorophenol.

B-5.3.7 Internal Standard Stock Solution — Dissolve 1 g of 2, 4 dibromophenol in 1 l of acetone. One millilitre of this solution contains 1 mg of dibromophenol.

B-5.3.8 Internal Standard Solution — Dilute 1 ml of the stock solution (B-5.3.7) with acetone to 100 ml. One millilitre of this solution contains 10 µg of dibromophenol.

B-5.4 Procedure

B-5.4.1 Determine the moisture content of the sample as given in 9 of IS 1060 (Part 1).

B-5.4.2 Weigh accurately about 1 g of the paper sample pieces up to two decimal places and put into a thimble. Extract with about 150 ml of acetone by Soxhlet extraction for 6 h. Filter the acetone extract, dry over anhydrous sodium sulphate, and evaporate under vacuum to a small volume approximately to 5 ml and cool.

B-5.4.3 Clean Up — Transfer the extract (B-5.4.2) to the silica gel packed column and elute with about 25 ml of *n*-hexane at the rate of 2 ml/min. Collect the eluent in a flask. Dry over anhydrous sodium sulphate and evaporate nearly to dryness.

B-5.4.4 Treat the residue (B-5.4.3) with 1 ml of acetic anhydride, and heat on a water bath for about 30 min. Remove the flask from the water bath and cool the acetylated product. Transfer the content in a separating funnel and add 10 ml of hexane and 5 ml distilled water. Shake well for 2 min and let the layers be separated. Collect the hexane layer, dry over anhydrous sodium sulphate and evaporate nearly to dryness. Cool for at least 10 min, add 1 ml of internal standard solution and adjust the volume to 5.0 ml with *n*-hexane.

B-5.4.5 Inject 2 µl of the solution into the Gas Chromatograph. Record the peak size in area and peak height units. If peak response exceeds linear range of the system, dilute the concentration of the extract and reanalyze.

B-5.4.6 Calibration — Prepare three calibration standards from the PCP standard solutions. Add 1 ml of internal standard solution and follow the steps as above (B-5.4.3 to B-5.4.5). Tabulate peak height or area responses against calculated equivalent mass of underivatized pentachlorophenol injected. Prepare a calibration curve.

B-5.5 Calculation — Determine the PCP content of the sample from the calibration graph using the following formula:

PCP content, mg/kg on dry matter =

$$\frac{A \times B \times V_i \times 100}{M \times C \times V_t \times 100 - X}$$

where

A = PCP content in µg from the graph;

B = total volume of hexane extract before derivatization, ml;

V_i = volume of eluent injected, ml;

M = mass of the paper sample taken for testing, g;

C = volume of hexane extract carried through derivatization, ml;

V_t = volume of total eluent, ml; and

X = moisture content, percent by mass.

B-6 DETERMINATION OF POLYCHLORINATED BIPHENYLS (PCBS)

B-6.1 Principle

PCB is extracted with boiling ethanolic potassium hydroxide solution. An aliquot of the extract is mixed with distilled water and subjected to extraction with hexane. The PCB content is determined quantitatively by GC-ECD by comparing the pattern of the peaks with the pattern of a suitable technical PCB.

B-6.2 Apparatus

B-6.2.1 Erlenmeyer Flask — 200 ml.

B-6.2.2 Water Bath

B-6.2.3 Separating Funnels — 60 ml and 100 ml.

B-6.2.4 Injection Syringes — 1 µl, 5 µl and 10 µl.

B-6.2.5 Gas Chromatograph with ECD — Capillary columns.

B-6.2.6 Glass Columns — Length 20 cm, internal diameter 12 mm filled with 5 cm of silica gel having particle size 63 µm × 200 µm.

B-6.3 Reagents

B-6.3.1 Ethanolic Potassium Hydroxide Solution — Prepare 1 N ethanolic potassium hydroxide solution by dissolving the required amount of potassium hydroxide in absolute ethanol that has been purified as follows:

Dissolve 1.5 g of silver nitrate in 3 ml of water and add it to one litre of alcohol. Dissolve 3 g of potassium hydroxide in the smallest amount of hot distilled water, cool, and add it to the silver nitrate solution. Shake thoroughly, allow the solution to stand for at least 24 h, filter and distill.

NOTE — Absolute alcohol denatured with 10 percent by volume of methanol may also be used.

B-6.3.2 *n*-Hexane

B-6.3.3 Sodium Sulphate Anhydrous

B-6.3.4 PCB Stock Solution — Dissolve 10 mg of any PCB technical in 100 ml of hexane. One ml of this solution contains 0.1 mg of PCB.

B-6.3.5 PCB Standard Solution — Dilute 10 ml of stock solution with hexane to 100 ml. One ml of this solution contains 0.01 mg of PCB.

B-6.3.6 Internal Standard Stock Solution — Dissolve 1 g of 2, 4 dibromophenol in 1 litre of *n*-hexane. One ml of this solution contains 1 mg of dibromophenol.

B-6.3.7 Internal Standard Solution — Dilute 1 ml of the stock solution (B-6.3.6) with hexane to 100 ml. One ml of this solution contains 10 µg of dibromophenol.

B-6.4 Procedure

B-6.4.1 Determine the moisture content of the sample as given in 9 of IS 1060 (Part 1).

B-6.4.2 Weigh accurately about 1 g of the paper sample pieces up to two decimal places and take into a 200 ml Erlenmeyer flask. Add 50 ml of ethanolic potassium hydroxide solution and heat under reflux condenser for 4 h, filter and dilute to the mark with alcohol in a 250 ml volumetric flask. Take an aliquot portion of the test solution in a separating funnel, add sufficient distilled water and 15 ml hexane. Shake well for 5 min and wait for 15 min. Collect the hexane phase.

B-6.4.3 Filter the hexane extract. Dry the filtrate over anhydrous sodium sulphate, and evaporate under

vacuum to approximately 5 ml. Take the residue for clean up.

B-6.4.4 Clean Up

Transfer the hexane extract (B-6.4.3) to the silica gel packed column and elute with about 25-ml of *n*-hexane at the rate of 2-ml/min. Collect the eluent in a flask and evaporate to a small volume. Add 1 ml of internal standard solution and made up to 10 ml with hexane.

B-6.4.5 Inject 2 µl of the solution to the gas chromatograph. From the peaks obtained PCB and Internal Standard are identified by their retention times as well as relative retention time.

B-6.4.6 Calibration

Prepare three calibration standards from the PCB standard solutions and follow the steps as above (B-6.4.3 to B-6.4.5). Tabulate peak height or area responses against calculated equivalent mass of underivatized pentachlorophenol injected. Prepare a calibration curve.

B-6.5 Calculation

Determine the PCB content of the sample from the calibration graph using the following formula:

$$\text{PCB content, mg/kg on dry matter} = \frac{A \times V_i \times 100}{M \times V_t \times (100 - X)}$$

where

A = PCB content in µg from the graph;

V_i = volume of eluent injected, ml;

M = mass of the paper sample taken for testing, g;

V_t = volume of total eluent, ml; and

X = moisture content, percent by mass.

ANNEX C

(Foreword)

COMMITTEE COMPOSITION

Paper Based Packaging Materials Sectional Committee, CHD 16

<i>Organization</i>	<i>Representative(s)</i>
Central Pulp and Paper Research Institute, Saharanpur	DR R. M. MATHUR (Chairman)
All India Federation of Master Printers, New Delhi	SHRI RANJAN KOTHARI SHRI SUBHAS HANDER (<i>Alternate</i>)
Ballarpur Industries Ltd, Yamuna Nagar	SHRI SHAMIM AHMED SHRI V. V. PATHARKAR (<i>Alternate</i>)
Central Forensic Science Laboratory, New Delhi	DR RAJINDER SINGH SHRI D. R. HANDA (<i>Alternate</i>)
Central Pulp and Paper Research Institute, Saharanpur	DR B. P. THAPLIYAL Ms RITA TANDON (<i>Alternate</i>)
Central Revenues Control Laboratory, New Delhi	SHRI R. P. SINGH
Century Pulp and Paper Mills, Dist Nainital	SHRI MANOJ GUPTA SHRI H. C. JOSHI (<i>Alternate</i>)
Directorate of Printing, Ministry of Urban Development, New Delhi	SHRI B. SAHOO
Department of Industrial Policy & Promotion, Ministry of Commerce & Industry, New Delhi	SHRI NAND LAL
DGS & D, New Delhi	SHRI H. M. RATHI SHRI RAMAN K. SHARMA (<i>Alternate</i>)
DGQA (Ministry of Defence), Kanpur DQA (Met & Explosives)	SHRI K. L. TRIPATHI SHRI C. KUJUR (<i>Alternate</i>)
Federation of Paper Traders' Associations of India, Delhi	SHRI SATYA PAL GUPTA SHRI NAROTTAM VYAS (<i>Alternate</i>)
Federation of Corrugated Box Manufacturers of India, New Delhi	SHRI SUNIL SETHI SHRI HARISH MADAN (<i>Alternate</i>)
Forest Research Institute, Dehradun	DR SANJAY NAITHANI
Hindustan Unilever Limited, Bengaluru	SHRI PRABUDDHA DASGUPTA SHRI HITESH SHENOY (<i>Alternate</i>)
Hindustan Paper Corporation Ltd, Kolkata	SHRI M. V. NARASIMHA RAO SHRI NABA K. GHOSH (<i>Alternate</i>)
Indian Paper Manufacturers Association, New Delhi	SHRI R. C. MALL DR S. V. SUBRAHMANYAM (<i>Alternate</i>)
India Security Press, Nasik	SHRI SUNIL TIWARI SHRI D. C. RAGHAV (<i>Alternate</i>)
Indian Agro & Recycled Paper Mills Association, New Delhi	SHRI P. G. MUKUNDAN DR M. PATEL (<i>Alternate</i>)
Indian Institute of Packaging, Mumbai	DR N. C. SAHA SHRI S. K. SARKAR (<i>Alternate</i>)
Indian Institute of Technology, Roorke	DR SATISH KUMAR DR S. P. SINGH (<i>Alternate</i>)
Indian Recycled Paper Mills Association, Delhi	SHRI R. C. RASTOGI

<i>Organization</i>	<i>Representative(s)</i>
Indian Newsprint Manufacturers Association, New Delhi	REPRESENTATIVE
Indian Pulp and Paper Technical Association, Saharanpur	SHRI M. B. S. NAIR SHRI N. K. GARG (<i>Alternate</i>)
J K Paper Ltd, New Delhi	SHRI S. C. MAJUMDAR SHRI S. K. CHATTERJEE (<i>Alternate</i>)
Kumarrappa National Handmade Paper Institute, Jaipur	SHRI G. HUSSAIN SHRI ASWINI SHARMA (<i>Alternate</i>)
NEPA Ltd, Nepanagar, Madhya Pradesh	SHRI S. K. MUTREJA SHRI NIAZI R. A. KHAN (<i>Alternate</i>)
North-East Institute of Science & Technology, Jorhat, Assam	DR T. GOSWAMI DR DIPUL KALITA (<i>Alternate</i>)
Parksons Packaging, Mumbai	SHRI RAMESH KEJRIWAL SHRI RANJAN SINHA (<i>Alternate</i>)
Pulp and Paper Research Institute, Orissa	DR J. C. PANIGRAHI SHRI D. K. TRIPATHY (<i>Alternate</i>)
Rollatainers Ltd, Haryana	REPRESENTATIVE
Security Paper Mill, Hoshangabad	SHRI B. B. DASH SHRI D. R. ROHILLA (<i>Alternate</i>)
Security Printing Press, Hyderabad	SHRI A. K. SRIVAYSTAVA SHRI D. D. MATHUR (<i>Alternate</i>)
Seshasayee Paper and Boards Ltd, Erode	SHRI A. K. MEHROTRA DR P. MARIMUTHU (<i>Alternate</i>)
Stationery Office, Govt of India, Kolkata	SHRI ATANU BANDOPADHYAY
The Mysore Paper Mills Ltd, Bengaluru	SHRI P. K. GARG, IAS SHRI N. P. PRABHU (<i>Alternate</i>)
TCPL Packaging Limited, Mumbai	SHRI SAKET KANORIA
VOICE, New Delhi	SHRI M. A. U. KHAN SHRI H. WADHWA (<i>Alternate</i>)
Whale Stationary Products Ltd, New Delhi	SHRI MUKESH GUPTA SHRI GAURAV GOEL (<i>Alternate</i>)
BIS Directorate General	SHRI E. DEVENDAR, SCIENTIST F AND HEAD (CHD) [REPRESENTING DIRECTOR GENERAL (<i>Ex-officio</i>)]

Member Secretary

SHRI K. K. PAUL
SCIENTIST 'E' (CHD), BIS

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 2016* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc No.: CHD 16 (1821).

Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002
Telephones: 2323 0131, 2323 3375, 2323 9402

Website: www.bis.gov.in

Regional Offices:

Telephones

Central	: Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110002	{ 2323 7617 2323 3841
Eastern	: 1/14 C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi KOLKATA 700054	{ 2337 8499, 2337 8561 2337 8626, 2337 9120
Northern	: Plot No. 4-A, Sector 27-B, Madhya Marg CHANDIGARH 160019	{ 265 0206 265 0290
Southern	: C.I.T. Campus, IV Cross Road, CHENNAI 600113	{ 2254 1216, 2254 1442 2254 2519, 2254 2315
Western	: Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400093	{ 2832 9295, 2832 7858 2832 7891, 2832 7892

Branches : AHMEDABAD. BENGALURU. BHOPAL. BHUBANESHWAR. COIMBATORE.
DEHRADUN. DURGAPUR. FARIDABAD. GHAZIABAD. GUWAHATI.
HYDERABAD. JAIPUR. JAMMU. JAMSHEDPUR. KOCHI. LUCKNOW.
NAGPUR. PARWANOO. PATNA. PUNE. RAIPUR. RAJKOT. VISAKHAPATNAM.

Published by BIS, New Delhi